


## Initial bare-bone system in Kremlin-Bicêtre hospital



- No applied field  
(5G from scanner at 10 m)
- No measurement of M

Gas delivery to subject :  
1 litre **plastic bag** (Tedlar®)

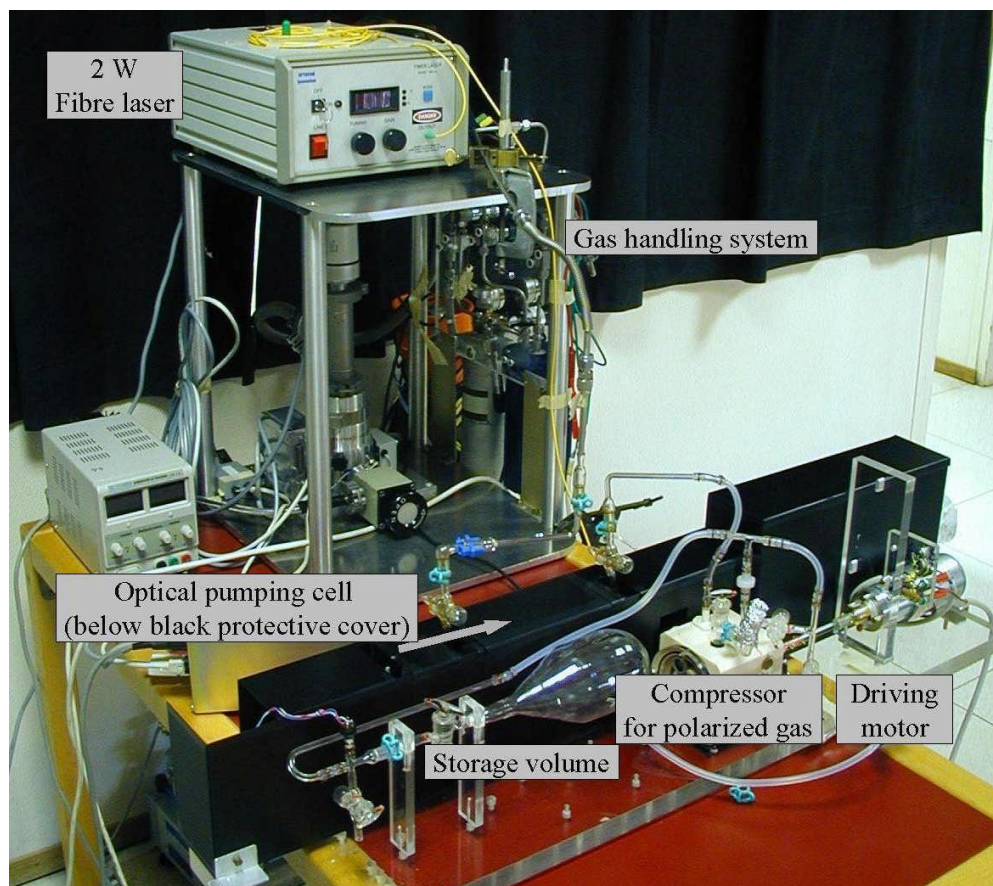